

p-Hydroxybenzoate Ester Analysis In Preservatives

1. Analytical Condition

YL 9100 Series QC Analyzer

Column : C18 (4.6*150mm, 5um)


Detector : UV/Vis 254nm

Flow rate : 1ml/min

Injection volume : 10 μ l

Mobile phase : ACN:Water:Acetic acid=55:44:1

2. Chromatogram

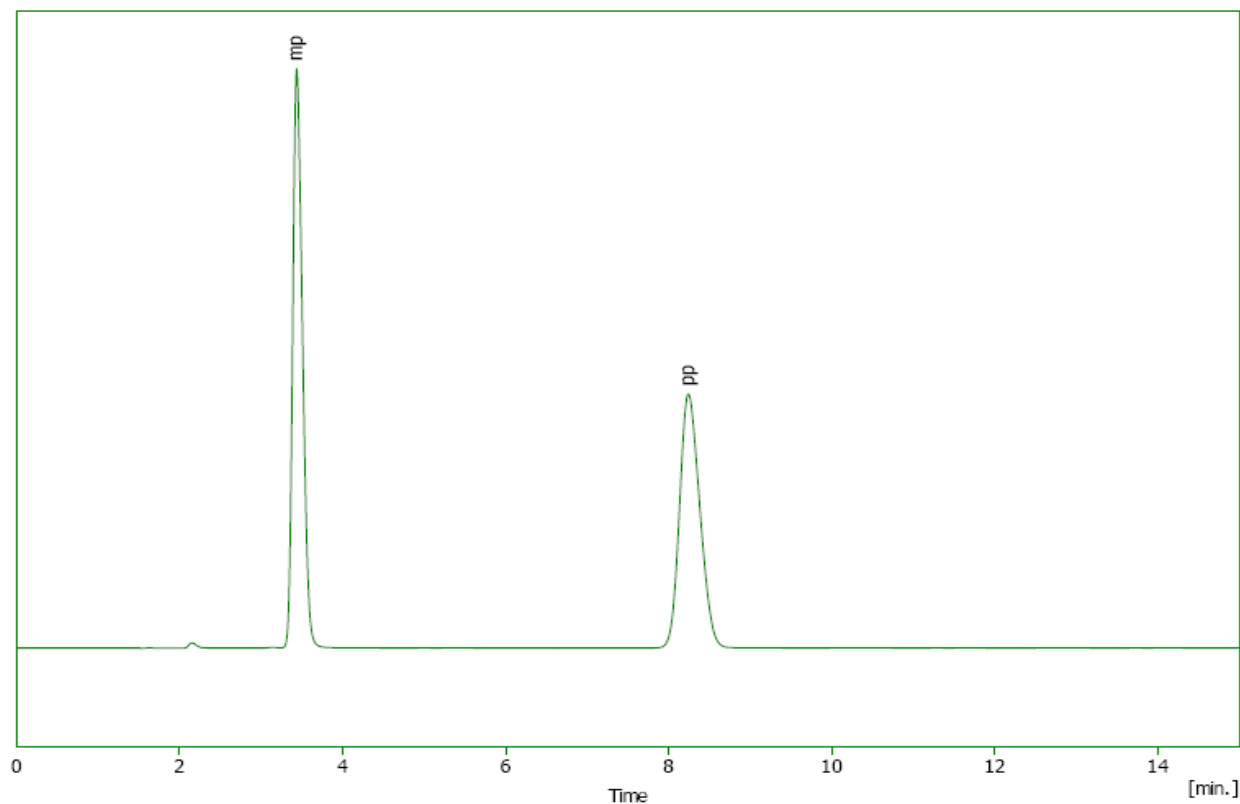

1. Methyl p-hydroxybenzoate

2. Propyl p-hydroxybenzoate