

# Sodium lactate Analysis

## 1. Analytical Condition

### YL 9100 Series HPLC

Mobile Phase : Water (0.15% H<sub>3</sub>PO<sub>4</sub>)

Flow Rate : 1.0ml/min

Column Oven : 40°C


Detector : UV/Vis 210nm

Column : C18 (4.6\*250mm, 5µm)


Injection Volume : 20µl sample loop

## 2. Chromatogram

Standard

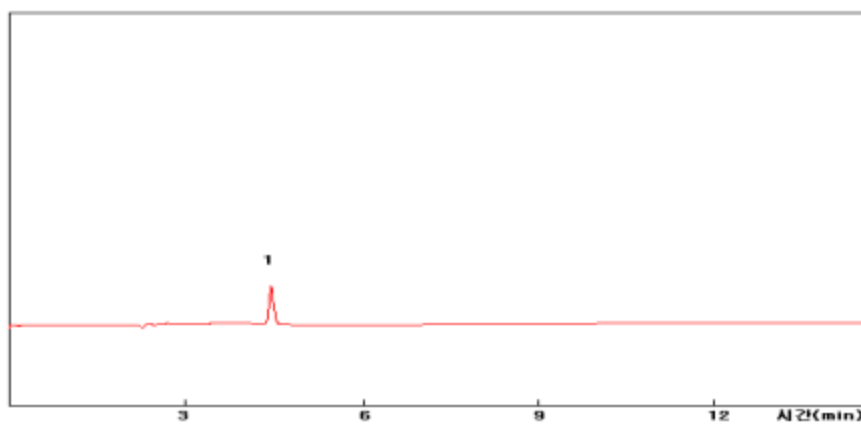

Example

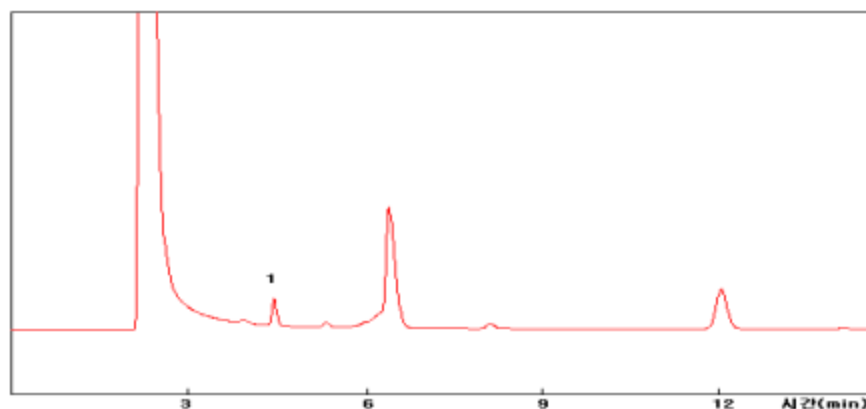

1. Sodium lactate

