

Pantothenic acid Analysis

1. Analytical Condition

YL 9100 HPLC

Column : Capcell pak C18(2.0 X 150mm, 5 μ m)


Detector : UV/Vis 200nm

Injection Volume : 5ul

Mobile Phase : [Triethylamine 5ml + H₃PO₄ 3ml]/Water 1L

Flow Rate : 0.4ml/min

2. Chromatogram

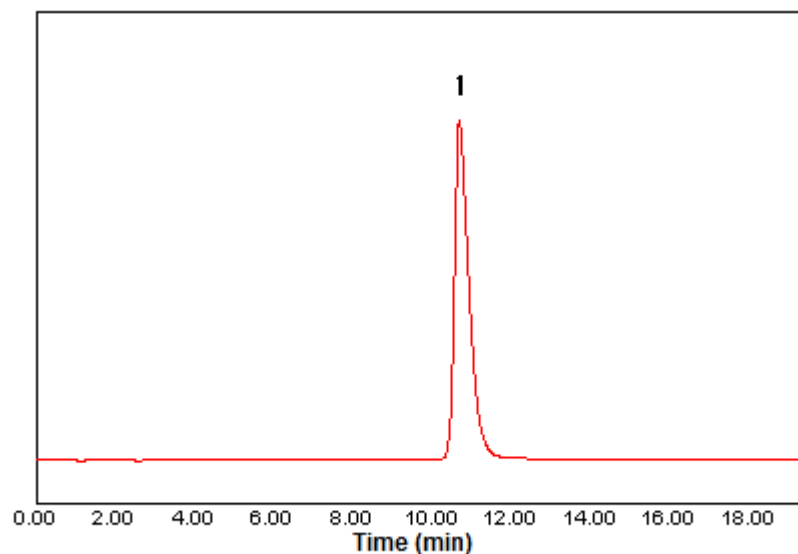

1. Pantothenic acid

