

Vitamin A Analysis

1. Analytical Condition

YL 9100 HPLC

Column : C18 (4.6 X 250mm, 5 μ m)


Detector : UV/Vis 325nm

Injection Volume : 20 μ l

Mobile Phase : ACN:MeOH=75:25

Flow Rate : 1ml/min

2. Chromatogram

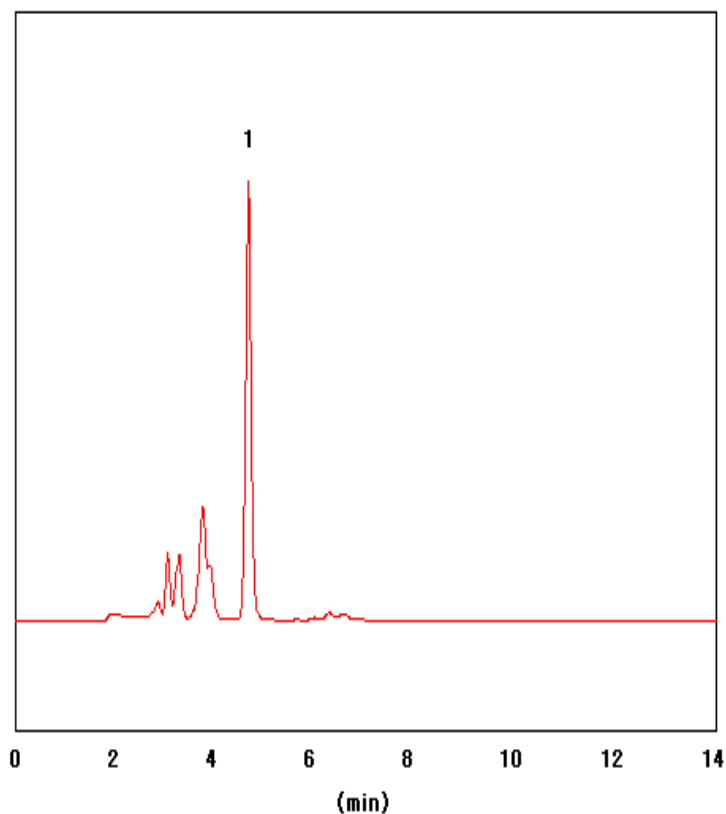

1. Vitamin A

